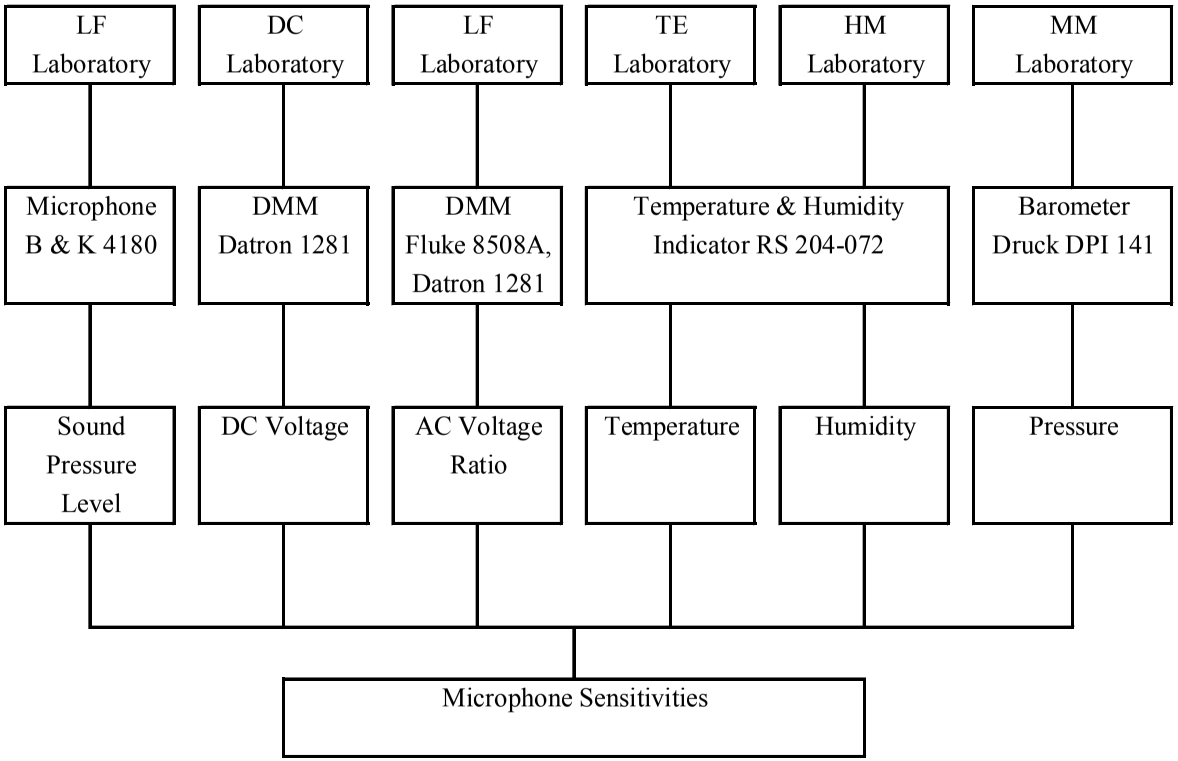Traceability of calibration of working grade microphones